

Imaging perfusion changes in oncological clinical applications by hyperspectral imaging: a literature review

Rok Hren^{1,2}, Gregor Sersa³, Urban Simoncic^{1,4}, Matija Milanic^{1,4}

¹ Faculty of Mathematics and Physics, University of Ljubljana, Ljubljana, Slovenia

² Institute of Mathematics, Physics, and Mechanics, Ljubljana, Slovenia

³ Institute of Oncology Ljubljana, Ljubljana, Slovenia

⁴ Jozef Stefan Institute, Ljubljana, Slovenia

Radiol Oncol 2022; 56(4): 420-429.

Received 27 October 2022

Accepted 2 November 2022

Correspondence to: Matija Milanic, Ph.D., Faculty of Mathematics and Physics, University of Ljubljana, Jadranska ulica 19, SI-1000 Ljubljana, Slovenia. E-mail matija.milanic@mf.uni-lj.si

Disclosure: No potential conflicts of interest were disclosed.

This is an open access article distributed under the terms of the CC-BY license (<https://creativecommons.org/licenses/by/4.0/>).

Background. Hyperspectral imaging (HSI) is a promising imaging modality that uses visible light to obtain information about blood flow. It has the distinct advantage of being noncontact, nonionizing, and noninvasive without the need for a contrast agent. Among the many applications of HSI in the medical field are the detection of various types of tumors and the evaluation of their blood flow, as well as the healing processes of grafts and wounds. Since tumor perfusion is one of the critical factors in oncology, we assessed the value of HSI in quantifying perfusion changes during interventions in clinical oncology through a systematic review of the literature.

Materials and methods. The PubMed and Web of Science electronic databases were searched using the terms "hyperspectral imaging perfusion cancer" and "hyperspectral imaging resection cancer". The inclusion criterion was the use of HSI in clinical oncology, meaning that all animal, phantom, ex vivo, experimental, research and development, and purely methodological studies were excluded.

Results. Twenty articles met the inclusion criteria. The anatomic locations of the neoplasms in the selected articles were as follows: kidneys (1 article), breasts (2 articles), eye (1 article), brain (4 articles), entire gastrointestinal (GI) tract (1 article), upper GI tract (5 articles), and lower GI tract (6 articles).

Conclusions. HSI is a potentially attractive imaging modality for clinical application in oncology, with assessment of mastectomy skin flap perfusion after reconstructive breast surgery and anastomotic perfusion during reconstruction of gastrointestinal conduit as the most promising at present.

Key words: hyperspectral imaging; oncology; resection; perfusion; cancer

Introduction

Cancer is the leading health problem in the world. Only in the EU-27 each year are 2.7 million people diagnosed with cancer, while 1.3 million die from the disease.¹ To deal with cancer, knowledge of cancer physiology is essential, where tissue perfusion is one of the most important physiological parameters. Perfusion of tumors is critical in their de-

velopment and growth. Early studies have shown that tumor growth is dependent on the development of vasculature that has the capacity to supply oxygen and nutrients to dividing tumor cells.² However, the vasculature is important not only for the supply of oxygen to tumors but also for the delivery of drugs into tumors.³ Finally, vasculature is also important for the response of tumors to surgery and other ablative techniques, such as ra-

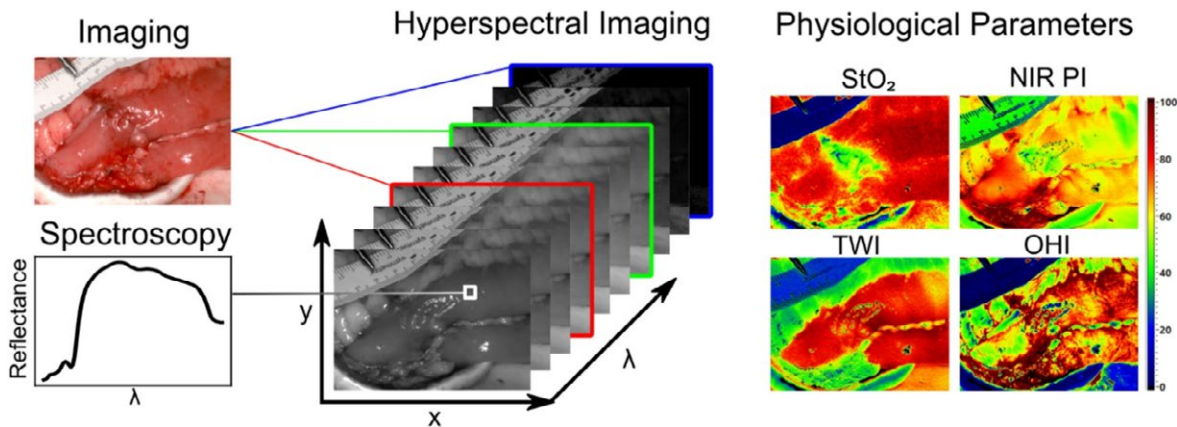


FIGURE 1. Structure and composition of hyperspectral images and physiological parameters derived from the images, which are typically displayed in false color.

NIR PI = near-infrared perfusion index; OHI = organ hemoglobin index; StO_2 = oxygen saturation of tissue; TWI = tissue water index

Taken from Pfahl et al.¹⁵ and reprinted with permission from the publisher.

diotherapy and thermal and nonthermal ablative techniques.^{4,5}

It was demonstrated that information about the tumor and healthy tissue perfusion can improve therapy outcome either by guiding tumor resection^{6,7} or monitoring the reperfusion of the resected tissues (e.g., anastomosis or tissue flaps).^{4,5} Conventional techniques for perfusion imaging in oncology are CT and MR imaging.¹⁰ CT perfusion imaging provides information on tissue hemodynamics by analyzing the first passage of an intravenous contrast bolus through the vessels. On the other hand, MR perfusion imaging utilizes either endogenous or exogenous tracers. In the latter case, it is based on following an injected bolus of contrast agent over time, which is then used to determine the perfusion characteristics of tissues. While both imaging techniques are promising, radiation exposure (CT), potential adverse events due to contrast (CT/MRI), limited access (MRI), high cost (MRI), and inability to scan at the bedside or in operating theater are disadvantages of the conventional techniques.¹⁰ To address these shortcomings, various imaging techniques, including optical imaging, have been explored for tissue perfusion imaging.^{11,12} In optical imaging, the optical contrast of tissues is intrinsically sensitive to tissue abnormalities, such as changes in oxygenation, blood concentration or scattering.^{13,14} These changes are characteristic of many tumors, since they include angiogenesis, hypervascularization, hypermetabolism, and hypoxia, making optical imaging techniques promising candidates for perfusion imaging in oncology.

Hyperspectral imaging (HSI) is an emerging optical imaging technique that uses light to obtain information about perfusion, or more specifically about oxygenation, water content or hemoglobin content of the tissue. The distinct advantage of HSI is that it is a noncontact, nonionizing, and noninvasive modality and does not require a contrast agent. HSI integrates conventional imaging and spectroscopy techniques by creating a set of images called a hypercube, which contains the spectral signature of the underlying tissue and in turn points to clinically relevant changes, such as angiogenesis or hypermetabolism. Figure 1 illustrates the structure and composition of hyperspectral images and physiological parameters derived from these images.

HSI was originally employed in remote sensing applications^{16,17} and then expanded into other fields, such as vegetation type and water source detection^{18,19}, wood product control²⁰, drug analysis²¹, food quality control²²⁻²⁵, artwork authenticity and restoration^{26,27}, and security²⁸. HSI is also an attractive modality in the medical field and has been successfully applied for the detection of various types of tumors, particularly in conjunction with histopathologic diagnosis.²⁹⁻³¹ HSI has, *inter alia*, already proven value in plastic and vascular surgery, where assessing perfusion predicted the outcome of healing processes in transplants and wounds.^{32,33}

How valuable HSI could be in quantifying perfusion changes during interventions in clinical oncology remains unclear, and to that end, we decided to systematically review the literature with

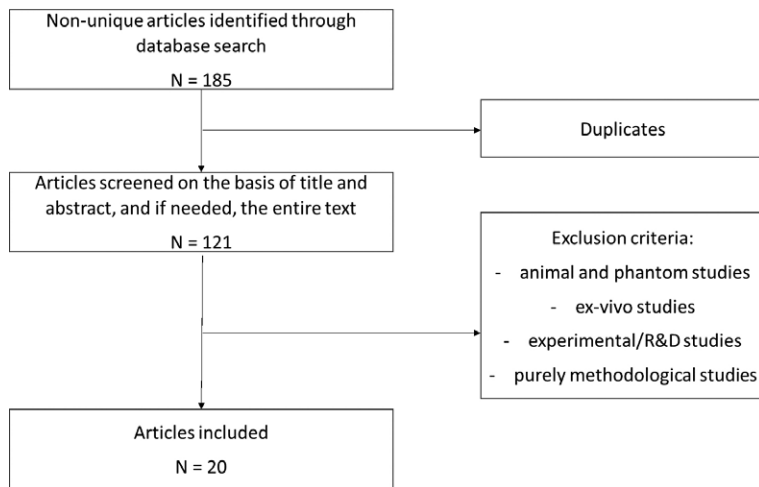


FIGURE 2. Flow diagram of the selection strategy.

the intention of exclusively focusing only on studies in which HSI was performed on patients in the clinical oncology setting.

Materials and methods

Two authors (R.H. and M.M.) conducted jointly – to preclude potential bias – a comprehensive literature search on October 3, 2022 through PubMed

and Web of Science electronic databases using the following search terms: »hyperspectral imaging perfusion cancer« and »hyperspectral imaging resection cancer«. No restrictions in publication date or language were imposed. The inclusion criterion was the application of the hyperspectral imaging modality in the oncological clinical setting, meaning that all animal and phantom, *ex vivo*, experimental, research and development, and purely methodological studies were excluded. Special care was taken that duplications were removed, both across databases and across studies; for example, if the study was first published in proceedings and later in the journal, then proceedings article was considered a nonprimary publication and therefore excluded. Studies were categorized with respect to the anatomical location of the tumors.

Results

A flow diagram of the selection strategy is shown in Figure 2; in total, 101 and 84 articles were found to be of interest in the PubMed and Web of Science databases, respectively. After excluding duplicates and applying the exclusion criteria, first considering the title and abstract, and next, if necessary, reading the entire article, 20 articles were identified for further analysis. The anatomical locations of tumors in the selected articles were as follows: kidneys (1 article), breasts (2 articles), eye (1 article), brain (4 articles), entire gastrointestinal (GI) tract (1 article), upper GI tract (5 articles) and lower GI tract (6 articles).




FIGURE 3. Images of the kidney depicting the percentage of HbO₂ as a function of color. A dark red represents high values while the yellows and greens indicate lower values.

Taken from Best *et al.*³⁴ and reprinted with permission from the publisher.

Kidneys

Pioneering effort in assessing perfusion by means of HSI in clinical oncology was the work of Best *et al.*³⁴ They applied modality to monitor renal oxygenation during partial nephrectomy using the parameter called the percentage of oxyhemoglobin (HbO₂) and categorized 26 patients into the preoperative groups of high (>75% HbO₂) and low (<75% HbO₂) oxygenation. Parameter HbO₂ has proven useful before, during and after the application of a clamp, with an example of the image presented in Figure 3. The study demonstrated that patients with low oxygenation had a statistically significant postoperative decline in estimated glomerular filtration rate. While further research is needed, HSI indicates potential for assessing susceptibility to renal ischemic injury in patients undergoing partial nephrectomy.

TABLE 1. Included articles reporting the use of hyperspectral imaging (HSI) to quantify perfusion changes in clinical applications in oncology

Reference	Year of publication	Number of patients	Oncologic intervention	System	Algorithm
Kidneys					
Best ³⁴	2013	26	Partial nephrectomy	DLP HSI, 520–645 nm	Supervised multivariate least squares regression
Eye					
Rose ³⁵	2018	8	Radiation retinopathy	Tunable laser, 520–620 nm with 5 nm steps	PHYSPEC software (Photon etc., Montreal, QC, Canada)
Breasts					
Chin ³⁶	2017	43	Skin response to radiation	OxyVu-2™ (Hypermed, Inc., Waltham, MA), 500–600 nm	The OxyVu-2™ software (Hypermed, Inc., Waltham, MA)
Pruimboom ⁸	2022	10	Mastectomy skin flap necrosis	TIVITA™ (Diaspective Vision GmbH, Am Salzhaff, Germany), 500–1000 nm with 5 nm step	TIVITA™ (Diaspective Vision GmbH, Am Salzhaff, Germany)
Brain					
Fabelo ³⁷	2018	22	Craniotomy for resection of intraaxial brain tumor	Hyperspec VNIR A-Series (HeadWall Photonics, Massachusetts, USA), 400–1000 nm	Spectral angle mapper
Fabelo ³⁸	2018	5	Craniotomy for resection of intraaxial brain tumor; all 5 patients with grade IV glioblastoma	As in Fabelo ³⁷	As in Fabelo ³⁷
Fabelo ³⁹	2019	6	Craniotomy for resection of intra-axial brain tumor; all 6 patients with grade IV glioblastoma	As in Fabelo ³⁷	As in Fabelo ³⁷
Fabelo ⁴⁰	2019	22	Craniotomy for resection of intraaxial brain tumor	As in Fabelo ³⁷	As in Fabelo ³⁷
Entire GI tract					
Jansen-Winkel ⁴¹ [Article in German]	2018	47	Gastrointestinal surgery with esophageal, gastric, pancreatic, small bowel or colorectal anastomoses	As in Pruimboom ⁸	As in Pruimboom ⁸
Upper GI tract					
Kohler ⁹	2019	22	Hybrid or open esophagectomy followed by reconstruction of gastric conduit	As in Pruimboom ⁸	As in Pruimboom ⁸
Moulla ⁴² [Article in German]	2020		Video presentation of hybrid esophagectomy	As in Pruimboom ⁸	As in Pruimboom ⁸
Schwandner ⁴³	2020	4	Hybrid esophagectomy followed by reconstructing gastric conduit	As in Pruimboom ⁸	As in Pruimboom ⁸
Hennig ⁴⁴	2021	13	Hybrid esophagectomy followed by reconstructing gastric conduit	As in Pruimboom ⁸	As in Pruimboom ⁸
Moulla ⁴⁵	2021	20	Pancreatoduodenectomy	As in Pruimboom ⁸	As in Pruimboom ⁸
Lower GI tract					
Jansen-Winkel ⁴⁶	2019	24	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸
Jansen-Winkel ⁴⁷	2020	32	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸
Pfahl ⁴⁸	2022	128	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸
Jansen-Winkel ⁴⁹	2021	54	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸
Jansen-Winkel ⁵⁰	2022	115	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸
Barberio ⁵¹	2022	52	Colorectal resection	As in Pruimboom ⁸	As in Pruimboom ⁸

GI = gastrointestinal

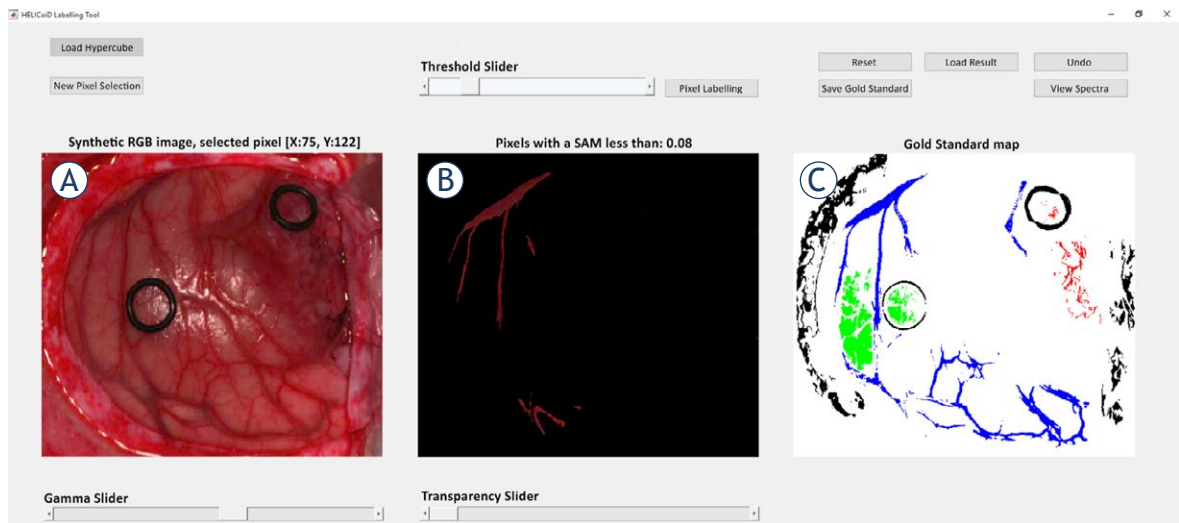


FIGURE 4. (A) Red-Green-Blue (RGB) representation of the imaged brain, including normal and tumor tissue. (B) Extraction of blood vessels from hyperspectral images using the spectral angle mapper algorithm (SAM). (C) Tissue classification map generated from hyperspectral images: tumor tissue is red, normal tissue is green, blood vessels are blue, and background is black.

Taken from Fabelo *et al.*³⁸ and reprinted with permission from the publisher.

Eye

In the study of Rose *et al.*³⁵, clinicians used Doppler spectral domain optical coherence tomography (SD-OCT) in 8 patients diagnosed with radiation retinopathy to measure total retinal blood flow, while retinal blood oxygen saturation was quantified by a specially designed HSI retinal camera. They found that blood flow in the retinopathy eye was significantly lower than that in the fellow eye, while arteriolar oxygen saturation and venular oxygen saturation were higher in the retinopathy eye than in the fellow eye. Unfortunately, researchers conducted no follow-up studies, in which they would further evaluate microvascular changes due to radiation-induced retinopathy.

Breasts

Chin *et al.*³⁶ studied a dose–response relationship between radiation exposure and oxygenated hemoglobin in 43 women undergoing breast-conserving therapy radiation. The authors concluded that HSI may prove useful as an objective measure of patients' skin response to radiation dose. However, they also noted that interpatient variability remains a challenge, as approximately 40% of the variability in change in oxygenated hemoglobin is accounted for by dose, 25% by individual woman, and 35% by causes that they could not identify.

Pruimboom *et al.*⁸ used HSI in a prospective clinical pilot study enrolling women with breast reconstruction and detected mastectomy skin flap necrosis in 3 out of 10 patients. Somewhat analogously to the study of Best *et al.*³⁴, they found that tissue oxygenation was statistically significantly lower in the group of patients who developed flap necrosis than in the group of patients who did not. It appears that HSI is specifically suited for the early detection of flap necrosis, which could in turn aid in the timely and accurate debridement of necrotic tissue. Future work should confirm the modality's potential also in identifying partial deep inferior epigastric artery perforator (DIEP) flap necrosis.

Brain

Fabelo *et al.*³⁷⁻⁴⁰ developed an intraoperative HSI acquisition system and were able to assemble an *in vivo* hyperspectral human brain image database with the overall goal of accurately delineating tumor tissue from normal brain tissue. As the brain tumor typically infiltrates the surrounding tissue, it is extremely difficult to identify the border; in addition, both overresection of adjacent normal brain tissue and leaving tumor tissue behind have detrimental impacts on the results of the surgery and patient outcomes, either adversely affecting the patient's quality of life or causing tumor progression.

The work of Fabelo *et al.* was performed as a part of the European Future and Emerging Technologies (FET) project HELICoiD (HypErspectraL Imaging Cancer Detection).

In their first methodological paper, they designed a special cancer detection algorithm utilizing spatial and spectral features of hyperspectral images from 5 patients with grade IV glioblastoma.³⁸ They demonstrated that it was possible to accurately discriminate between normal tissue, tumor tissue, blood vessels and background by generating classification and segmentation maps in surgical time during neurosurgical operations, as shown in Figure 4.

In their second methodological paper³⁹, they used data from 6 patients with grade IV glioblastoma and applied improved algorithms to create maps, in which the parenchymal area of the brain could be delineated; an overall average accuracy of 80% was achieved.

Their HSI system was systematically assessed at two clinical institutions enrolling 22 patients, and researchers found that results relevant for surgeons were obtained within 15 to 70 seconds.⁴⁰ They also made available to the public this first *in vivo* hyperspectral human brain image database specifically designed for cancer detection. While authors were hopeful in their conclusion that HSI could facilitate brain tumor surgeries, no further studies beyond 2019 were published.

HSI files from the studies by Fabelo and co-workers are available from <http://hsibraindatabase.iuima.ulpgc.es> database.

Entire gastrointestinal tract

During the past 3 years, the main focus of applying HSI in clinical oncology has been in the domain of the gastrointestinal tract, or more specifically, addressing anastomotic insufficiency, which is one of the most serious postsurgery complications of reconstructing the gastrointestinal conduit. As anastomotic healing fundamentally depends on adequate perfusion, HSI could be a suitable modality in assessing anastomotic perfusion in clinical practice. In a pilot study, Jansen-Winkeln *et al.*⁴¹ collected hyperspectral images in 47 patients who underwent gastrointestinal oncologic resection followed by esophageal, gastric, pancreatic, small bowel or colorectal anastomoses. The recorded hyperspectral images were analyzed to extract the following specific physiological tissue parameters, which were deemed characteristic for perfusion changes at the sites of anastomoses: oxygen satu-

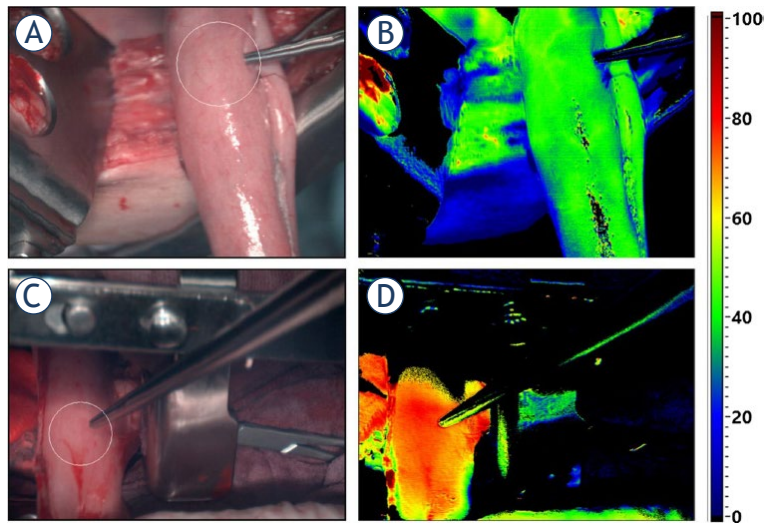


FIGURE 5. Comparison of Red-Green-Blue (RGB) images and near-infrared perfusion index (NIR PI) images recorded in a patient with (A, B) and without postoperative anastomotic insufficiency (C, D).

Taken from Köhler *et al.*⁹ and reprinted with permission from the publisher.

ration of the tissue (StO_2), organ hemoglobin index (OHI), near-infrared perfusion index (NIR-PI), and tissue water index (TWI); the most clinically relevant appeared to be StO_2 . They concluded that intraoperative HSI provided a noncontact, noninvasive modality, which enabled real-time analysis of potential anastomotic leakage without the use of a contrast medium. Their group followed their initial work with several studies focusing on the upper and lower gastrointestinal tract, respectively, described in more detail below.

Upper gastrointestinal tract

Köhler *et al.*⁹ applied intraoperative HSI in 22 patients during esophagectomy to the tip of the gastric tube, which later became esophagogastric anastomosis; they compared physiological HSI parameters (StO_2 , OHI, NIR PI and TWI) in 14 patients who underwent laparoscopic gastrolisis and ischemic conditioning of the stomach with those in 8 patients without pretreatment. They noted that the values of physiological HSI parameters were higher in patients with ischemic preconditioning; however, only StO_2 exhibited weak statistical significance. In a single patient who developed anastomotic insufficiency of the intrathoracic esophagogastric anastomosis, all physiological HSI parameters were substantially lower than those in



FIGURE 6. Hyperspectral imaging (HSI) acquisition system in the operating room. Hyperspectral images were acquired within a few seconds with physiologic HSI parameters displayed in false colors.

Taken from Moulla *et al.*⁴⁵ and reprinted with permission from the publisher.

other patients. Figure 5 compares the *NIR PI* image recorded in this patient with the corresponding image taken in the patient without postoperative anastomotic leakage. Hybrid esophagectomy along with intraoperative HSI used in the paper of Köhler *et al.*⁹ was presented as a video article by Moulla *et al.*⁴², while another clinical group⁴³ corroborated the findings of Köhler *et al.*⁹ by reporting a case study including four patients.

Hennig *et al.*⁴⁴ continued the systematic evaluation of the capabilities of intraoperative HSI in 13 consecutive patients who underwent hybrid esophagectomy and reconstruction of the gastric conduit. Researchers also decided to use both intraoperative HSI and fluorescence imaging with indocyanine green (FI-ICG) to define the optimal position of anastomosis. While there are no threshold values yet established to define adequately and insufficiently perfused tissues, they decided that HSI physiological parameter StO_2 at $>75\%$ determined the well-perfused area. It was noteworthy that imaging modalities recorded simultaneously in 10 out of 13 patients identified the perfusion border zone more peripherally than the one desig-

nated subjectively by the surgeon. While HSI and FI-ICG may complement each other as intraoperative modalities, Hennig *et al.*⁴⁴ were of the opinion that HSI may be advantageous due to “the lower costs, noninvasiveness, and lack of contraindications”.

Moulla *et al.*⁴⁵ expanded oncological clinical applications in the domain of pancreatic surgery. Hyperspectral images were recorded during pancreatoduodenectomy in 20 consecutive patients before and after gastroduodenal artery clamping. In this pilot study, they were able to detect by the means of physiologic HSI parameter StO_2 improvement in liver perfusion after median acute ligament division in one patient with celiac artery stenosis. The HSI acquisition system in the operating room is shown in Figure 6.

Lower gastrointestinal tract

Jansen-Winkel *et al.*⁹ applied intraoperative HSI in 24 patients to define the transection line during colorectal surgery. They found that the transection line subjectively delineated by the surgeon

deviated from the border line determined by HSI; in 13 patients subjectively, planned resection was up to 13 mm too distal in the poorly perfused area, while in 11 patients, it was too far in the well-perfused area. Similar to esophagectomy⁴⁴, intraoperative HSI has shown potential in determining the optimal anastomotic area during colorectal surgery.

Jansen-Winkeln *et al.*⁴⁷ applied further intraoperative HSI along with FI-ICG in 32 consecutive patients undergoing colorectal resection and concluded that both modalities provided similar information in specifying the perfusion border zone and could complement each other. To optimize the performance of both modalities, Pfahl *et al.*⁴⁸ constructed the combined FI-ICG and HSI system, which was tested in 128 patients.

In another study⁴⁹, Jansen-Winkeln *et al.* imaged colorectal tumors in 54 consecutive patients during colorectal resections and found that HSI used in combination with a neural-network algorithm was able to classify cancer or adenomatous margins around the central tumor with a sensitivity of 86% and a specificity of 95%. Recently, they published a large study⁵⁰ enrolling 115 patients who underwent colorectal resection to systematically assess the feasibility of HSI in quantifying tissue perfusion, and in accordance with a smaller patient series, they found that “well-perfused areas were clearly distinguishable from the less perfused ones only after one minute”^{46,47} Similar conclusions were reached in a group of 52 patients undergoing colorectal surgery by Barberio *et al.*⁵¹, who also found that the physiological HSI parameter StO_2 was significantly lower in patients receiving neoadjuvant radio/chemotherapy than in other oncological patients. Figure 7 illustrates the usefulness of HSI in establishing the transection line during colorectal surgery.

Discussion

Based on this literature review, the following inferences could be made: HSI is still finding its place in oncological clinical applications with the assessment of (i) mastectomy skin flap perfusion after breast reconstructive surgery⁸ and (ii) anastomotic perfusion during reconstruction of gastrointestinal conduit^{9,44,45,48-50} as the most promising. However, caution needs to be advised because recently much research has been done in the arena of using HSI during brain surgery for glioblastoma, yet this clinical effort has not been sustained.




FIGURE 7. Usefulness of hyperspectral imaging (HSI) in establishing transection line during colorectal surgery. The Red-Green-Blue (RGB) image (A) and StO_2 map (B) show a patient in whom the clinical transection line (continuous line in black) and HSI transection line (dotted line in blue) were aligned; (C) and (D) show the RGB image and StO_2 map, respectively, of a patient in whom the clinical transection line deviated from the HSI transection line.

Taken from Barberio *et al.*⁵¹ and reprinted with permission from the publisher.

In addition, the need for an obvious expansion of the study of Pruijboom *et al.*⁸ to a larger patient group, which would also include cases of DIEP flap necrosis, a meaningful and robust establishment of cutoff values for physiological HSI parameters is mandatory if HSI is to retain its clinical appeal. In their study, oxygen saturation of tissue StO_2 appeared to be the most useful HSI index, and the cut-off value of 36.3% predicting tissue necrosis was found; this value was close to that defined by a pilot study⁵² enrolling mostly nononcological patients (19 out of 22), in which the values of both StO_2 and $NIR PI$ above 40% indicated regular healing without any revision surgery; furthermore, operators in that study noted that HSI was superior to assessments based on clinical and Doppler ultrasound monitoring both in accuracy and speed. It is worthwhile to emphasize that HSI parameters are in general easy to follow by the operator as they are visualized as false-colour images (Figure 1).

When evaluating applications of HSI in assessing anastomotic perfusion during reconstructing gastrointestinal conduits, two main challenges become apparent: (i) the first challenge is, as in the case of breast reconstructive surgery, related to the establishment of a clear cutoff value indicating

adequate tissue perfusion so that the operator can convincingly identify the optimal anastomosis area; (ii) the second challenge is related to HSI being limited to open surgery due to the large size of the HSI camera. The first challenge will need to be approached by enrolling progressively larger patient groups undergoing various oncological surgical interventions. It appears that the group of Jansen-Winkeln *et al.*^{48,50} is already moving in this direction by conducting progressively larger clinical studies. However, with the application of neural networks, requirements for cohort sizes become far higher but could also be partially satisfied with the data augmentation. The second challenge has been recently addressed by the same group¹⁵, with *ex vivo* testing of laparoscopic HSI camera and a highlight that the clinical trial with minimally invasive HSI has commenced already.

Comparison of HSI and FI-ICG^{44,47,48} revealed similar results in defining the perfusion border of anastomosis, while both modalities were documented to be reliable, fast, and intuitive. Even if HSI is completely noninvasive, injection of ICG rarely provokes allergic reactions. Since there is a potential for each of the two modalities to contribute complementary information, it is not surprising that Pfahl *et al.*⁴⁸ constructed a combined HSI and FI-ICG recording system.

In conclusion, HSI is at this stage emerging as an attractive imaging modality to quantify perfusion in oncological patients. Hopefully, a larger number of clinical sites will initiate clinical trials to address the challenges, which still preclude the final acceptance of this promising imaging technique in the oncological clinical setting.

Acknowledgment

This work was financially supported by the state budget by the Slovenian Research Agency, research grant no. J3-3083 and research program no. P3-0003, P3-0307, and P1-0389.

We would like to thank Dr. Ivan Stajduhar from University of Rijeka, Faculty of Engineering for his technical support in preparing Figures for publishing.

References

- European Commission. ECIS - European cancer information system [Internet]. 2022. [cited 2022 Oct 15]. Available from: <https://ecis.jrc.ec.europa.eu/>
- Folkman J. Role of angiogenesis in tumor growth and metastasis. *Semin Oncol* 2002; **29**: 15-8. doi: 10.1053/sonc.2002.37263
- Stylianopoulos T, Munn LL, Jain RK. Reengineering the tumor vasculature: improving drug delivery and efficacy. *Trends Cancer* 2018; **4**: 258-9. doi: 10.1016/j.trecan.2018.02.010
- Sersa G, Ursic K, Cemazar M, Heller R, Bosnjak M, Campana LG. Biological factors of the tumour response to electrochemotherapy: review of the evidence and a research roadmap. *Eur J Surg Oncol* 2021; **47**: 1836-46. doi: 10.1016/j.ejso.2021.03.229
- Kanthou C, Tozer G. Targeting the vasculature of tumours: combining VEGF pathway inhibitors with radiotherapy. *Brit J Radiol* 2019; **92**: 20180405. doi: 10.1259/bjir.20180405
- Popiel B, Gupta D, Misra S. Value of an intraoperative real time tissue perfusion assessment system following a nipple-sparing radical mastectomy for advanced breast cancer. *Int J Surg Case Rep* 2014; **5**: 30-3. doi: 10.1016/j.ijscr.2013.11.007
- Crawford T, Moshnikova A, Roles S, Weerakkody D, DuPont M, Carter LM, et al. pHLIP ICG for delineation of tumors and blood flow during fluorescence-guided surgery. *Sci Rep* 2022; **10**: 18356. doi: 10.1038/s41598-020-75443-5
- Pruimboom T, Lindelauf AAMA, Felli E, Sawor JH, Deliaert AEK, van der Hulst RRWJ, et al. Perioperative hyperspectral imaging to assess mastectomy skin flap and DIEP flap perfusion in immediate autologous breast reconstruction: a pilot study. *Diagnostics* 2022; **12**: 184. doi: 10.3390/diagnostics12010184
- Köhler H, Jansen-Winkeln B, Maktabi M, Barberio M, Takoh J, Holfert N, et al. Evaluation of hyperspectral imaging (HSI) for the measurement of ischemic conditioning effects of the gastric conduit during esophagectomy. *Surg Endosc* 2019; **33**: 3775-82. doi: 10.1007/s00464-019-06675-4
- Trinh A, Wintermark M, Iv M. Clinical review of computed tomography and MR perfusion imaging in neuro-oncology. *Radiol Clin North Am* 2021; **59**: 323-34. doi: 10.1016/j.rcl.2021.01.002
- van Manen L, Handgraaf HJM, Diana M, Dijkstra J, Ishizawa T, Vahrmeijer AL, et al. A practical guide for the use of indocyanine green and methylene blue in fluorescence-guided abdominal surgery. *J Surg Oncol* 2018; **118**: 283-300. doi: 10.1002/jso.25105
- Wiesinger I, Jung F, Jung EM. Contrast-enhanced ultrasound (CEUS) and perfusion imaging using VueBox®. *Clin Hemorheol Microcirc* 2021; **78**: 29-40. doi: 10.3233/CH-201040
- Jacques SL. Optical properties of biological tissues: a review. *Phys Med Biol* 2013; **58**: R37-61. doi: 10.1088/0031-9155/58/11/R37
- Bashkatov AN, Genina EA, Tuchin VV. Optical properties of skin, subcutaneous, and muscle tissues: a review. *J Innov Opt Health Sci* 2011; **04**: 9-38. doi: 10.1142/S1793545811001319
- Pfahl A, Köhler H, Thomaßen MT, Maktabi M, Bloße AM, Mehdorn M, et al. Clinical evaluation of a laparoscopic hyperspectral imaging system. *Surg Endosc* 2022; **36**: 7794-9. doi: 10.1007/s00464-022-09282-y
- Goetz AFH, Vane G, Solomon JE, Rock BN. Imaging spectrometry for earth remote sensing. *Science* 1985; **228**: 1147-53. doi: 10.1126/science.228.4704.1147
- Selci S. The future of hyperspectral imaging. *J Imaging* 2019; **5**: 84. doi: 10.3390/jimaging5110084
- Govender M, Chetty K, Bulcock H. A review of hyperspectral remote sensing and its application in vegetation and water resource studies. *Water SA* [Internet]. 2007; **33**: 145-51. [cited 2022 Oct 8]. Available from: <http://www.ajol.info/index.php/wsa/article/view/49049>
- Castro-Esau K. Discrimination of lianas and trees with leaf-level hyperspectral data. *Remote Sens Environ* 2004; **90**: 353-72. doi: 10.1016/j.rse.2004.01.013
- Schimleck L, Ma T, Inagaki T, Tsuchikawa S. Review of near infrared hyperspectral imaging applications related to wood and wood products. *Appl Spectrosc Rev* 2022; **1**-25. doi: 10.1080/05704928.2022.2098759
- Puchert T, Lochmann D, Menezes JC, Reich G. Near-infrared chemical imaging (NIR-CI) for counterfeit drug identification—A four-stage concept with a novel approach of data processing (Linear Image Signature). *J Pharm Biomed Anal* 2010; **51**: 138-45. doi: 10.1016/j.jpba.2009.08.0221
- Feng YZ, Sun DW. Application of hyperspectral imaging in food safety inspection and control: a review. *Crit Rev Food Sci Nutr* 2012; **52**: 1039-58. doi: 10.1080/10408398.2011.651542

23. Huang H, Liu L, Ngadi M. Recent developments in hyperspectral imaging for assessment of food quality and safety. *Sensors* 2014; **14**: 7248-76. doi: 10.3390/s140407248
24. Gowen A, Odonnell C, Cullen P, Downey G, Frias J. Hyperspectral imaging – an emerging process analytical tool for food quality and safety control. *Trends Food Sci Technol* 2007; **18**: 590-8. doi: 10.1016/j.tifs.2007.06.001
25. Soni A, Dixit Y, Reis MM, Brightwell G. Hyperspectral imaging and machine learning in food microbiology: Developments and challenges in detection of bacterial, fungal, and viral contaminants. *Comp Rev Food Sc Food Safe* 2022; **21**: 3717-45. doi: 10.1111/1541-4337.12983
26. Balas C, Epitropou G, Tsapras A, Hadjinicolaou N. Hyperspectral imaging and spectral classification for pigment identification and mapping in paintings by El Greco and his workshop. *Multimed Tools Appl* 2018; **77**: 9737-51. doi: 10.1007/s11042-017-5564-2
27. Sandak J, Sandak A, Legan L, Retko K, Kavčić M, Kosel J, et al. Nondestructive evaluation of heritage object coatings with four hyperspectral imaging systems. *Coatings* 2021; **11**: 244. doi: 10.3390/coatings11020244
28. Yuen PW, Richardson M. An introduction to hyperspectral imaging and its application for security, surveillance and target acquisition. *Imaging Sci J* 2010; **58**: 241-53. doi: 10.1179/174313110X12771950995716
29. Ortega S, Fabelo H, Camacho R, de la Luz Plaza M, Callicó GM, Sarmiento R. Detecting brain tumor in pathological slides using hyperspectral imaging. *Biomed Opt Express* 2018; **9**: 818. doi: 10.1364/BOE.9.000818
30. Ortega S, Fabelo H, Iakovidis D, Koulaouzidis A, Callico G. Use of hyperspectral/multispectral imaging in gastroenterology. Shedding some – different – light into the dark. *J Clin Med* 2019; **8**: 36. doi: 10.3390/jcm8010036
31. Ma L, Halicek M, Zhou X, Dormer JD, Fei B. Hyperspectral microscopic imaging for automatic detection of head and neck squamous cell carcinoma using histologic image and machine learning. In: Tomaszewski JE, Ward AD, editors. *Medical Imaging 2020: Digital Pathology* [Internet]. Houston, United States: SPIE; 2020. p. 31. [cited 2022 Oct 8]. Available from: <https://www.spiedigitallibrary.org/conference-proceedings-of-spie/11320/2549369/Hyperspectral-microscopic-imaging-for-automatic-detection-of-head-and-neck/10.1117/12.2549369.full>
32. Keller A. A new diagnostic algorithm for early prediction of vascular compromise in 208 microsurgical flaps using tissue oxygen saturation measurements. *Ann Plast Surg* 2009; **62**: 538-43. doi: 10.1097/SAP.0b013e3181a47ce8
33. Jafari-Saraf L, Wilson SE, Gordon IL. Hyperspectral image measurements of skin hemoglobin compared with transcutaneous PO2 measurements. *Ann Vasc Surg* 2012; **26**: 537-48. doi: 10.1016/j.avsg.2011.12.002
34. Best SL, Thapa A, Jackson N, Olweny E, Holzer M, Park S, et al. Renal oxygenation measurement during partial nephrectomy using hyperspectral imaging may predict acute postoperative renal function. *J Endourol* 2013; **27**: 1037-40. doi: 10.1089/end.2012.0683
35. Rose K, Krema H, Durairaj P, Dangboon W, Chavez Y, Kulasekara SI, et al. Retinal perfusion changes in radiation retinopathy. *Acta Ophthalmol* 2018; **96**: e727-31. doi: 10.1111/aos.13797
36. Chin MS, Siegel-Reamer L, FitzGerald GA, Wyman A, Connor NM, Lo YC, et al. Association between cumulative radiation dose, adverse skin reactions, and changes in surface hemoglobin among women undergoing breast conserving therapy. *Clin Transl Radiat Oncol* 2017; **4**: 15-23. doi: 10.1016/j.ctro.2017.03.003
37. Fabelo H, Ortega S, Lazcano R, Madroñal D, M. Callicó G, Juárez E, et al. An intraoperative visualization system using hyperspectral imaging to aid in brain tumor delineation. *Sensors* 2018; **18**: 430. doi: 10.3390/s18020430
38. Fabelo H, Ortega S, Ravi D, Kiran BR, Sosa C, Bulters D, et al. Spatio-spectral classification of hyperspectral images for brain cancer detection during surgical operations. Fred AL, editor. *PLoS ONE* 2018; **13**: e0193721.
39. Fabelo H, Halicek M, Ortega S, Shahedi M, Szolna A, Piñero J, et al. Deep learning-based framework for in vivo identification of glioblastoma tumor using hyperspectral images of human brain. *Sensors* 2019; **19**: 920. doi: 10.3390/s19040920
40. Fabelo H, Ortega S, Szolna A, Bulters D, Pineiro JF, Kabwama S, et al. In-vivo hyperspectral human brain image database for brain cancer detection. *IEEE Access* 2019; **7**: 39098-116. doi: 10.1109/ACCESS.2019.2904788
41. Jansen-Winkeln B, Maktabi M, Takoh JP, Rabe SM, Barberio M, Köhler H, et al. [Hyperspectral imaging in gastrointestinal anastomoses]. [German]. *Chirurg* 2018; **89**: 717-25.
42. Moulla Y, Reifenrath M, Rehmet K, Niebisch S, Jansen-Winkeln B, Sucher R, et al. [Hybrid esophagectomy with intraoperative hyperspectral imaging: video contribution]. [German]. *Chirurg* 2020; **91**(S1): 1-12.
43. Schwandner F, Hinz S, Witte M, Philipp M, Schafmayer C, Grambow E. Intraoperative assessment of gastric sleeve oxygenation using hyperspectral imaging in esophageal resection: a feasibility study. *Visc Med* 2021; **37**: 165-70. doi: 10.1159/000509304
44. Hennig S, Jansen-Winkeln B, Köhler H, Knospe L, Chalopin C, Maktabi M, et al. Novel intraoperative imaging of gastric tube perfusion during oncologic esophagectomy – a pilot study comparing hyperspectral imaging (HSI) and fluorescence imaging (FI) with indocyanine green (ICG). *Cancers* 2021; **14**: 97. doi: 10.3390/cancers14010097
45. Moulla Y, Buchloh DC, Köhler H, Rademacher S, Denecke T, Meyer HJ, et al. Hyperspectral Imaging (HSI) – A new tool to estimate the perfusion of upper abdominal organs during pancreatoduodenectomy. *Cancers* 2021; **13**: 2846. doi: 10.3390/cancers13112846
46. Jansen-Winkeln B, Holfert N, Köhler H, Moulla Y, Takoh JP, Rabe SM, et al. Determination of the transection margin during colorectal resection with hyperspectral imaging (HSI). *Int J Colorectal Dis* 2019; **34**: 731-9. doi: 10.1007/s00384-019-03250-0
47. Jansen-Winkeln B, Germann I, Köhler H, Mehdorn M, Maktabi M, Sucher R, et al. Comparison of hyperspectral imaging and fluorescence angiography for the determination of the transection margin in colorectal resections – a comparative study. *Int J Colorectal Dis* 2021; **36**: 283-91. doi: 10.1007/s00384-020-03755-z
48. Pfahl A, Radmacher GK, Köhler H, Maktabi M, Neumuth T, Melzer A, et al. Combined indocyanine green and quantitative perfusion assessment with hyperspectral imaging during colorectal resections. *Biomed Opt Express* 2022; **13**: 3145. doi: 10.1364/BOE.452076
49. Jansen-Winkeln B, Barberio M, Chalopin C, Schierle K, Diana M, Köhler H, et al. Feedforward artificial neural network-based colorectal cancer detection using hyperspectral imaging: a step towards automatic optical biopsy. *Cancers* 2021; **13**: 967. doi: 10.3390/cancers13050967
50. Jansen-Winkeln B, Dvorak M, Köhler H, Maktabi M, Mehdorn M, Chalopin C, et al. Border line definition using hyperspectral imaging in colorectal resections. *Cancers* 2022; **14**: 1188. doi: 10.3390/cancers14051188
51. Barberio M, Lapergola A, Benedicenti S, Mita M, Barbieri V, Rubichi F, et al. Intraoperative bowel perfusion quantification with hyperspectral imaging: a guidance tool for precision colorectal surgery. *Surg Endosc* [Internet]. 14 July 2022. [cited 2022 Oct 8]. Available from: <https://link.springer.com/10.1007/s00464-022-09407-3>
52. Kohler LH, Köhler H, Kohler S, Langer S, Nuwayhid R, Gockel I, et al. Hyperspectral imaging (HSI) as a new diagnostic tool in free flap monitoring for soft tissue reconstruction: a proof of concept study. *BMC Surg* 2021; **21**: 222. doi: 10.1186/s12893-021-01232-0